



# Quality Control




Dilution	1	2	3	4	5	6	7
Concentration	$1 \times 10^{-1}$	$1 \times 10^{-2}$	$1 \times 10^{-3}$	$1 \times 10^{-4}$	$1 \times 10^{-5}$	$1 \times 10^{-6}$	$1 \times 10^{-7}$
N° of copies	$1 \times 10^7$	$1 \times 10^6$	$1 \times 10^5$	$1 \times 10^4$	$1 \times 10^3$	$1 \times 10^2$	$1 \times 10^1$



Target Name	Sample Name	Reporter	Ct values
<i>Lymphocytic choriomeningitis</i>	1	FAM	12,93
	2	FAM	15,53
	3	FAM	19,72
	4	FAM	23,39
	5	FAM	26,34
	6	FAM	30,79
	7	FAM	33,39
	Negative Control	FAM	Undetermined

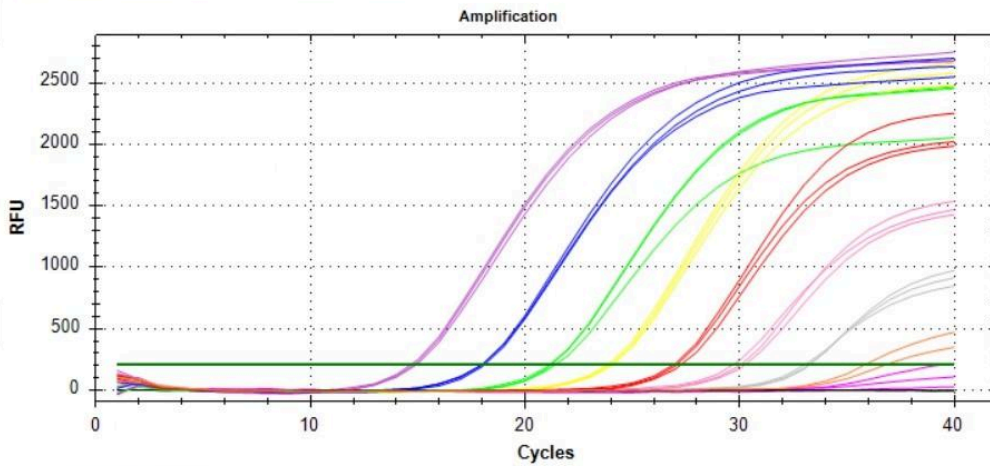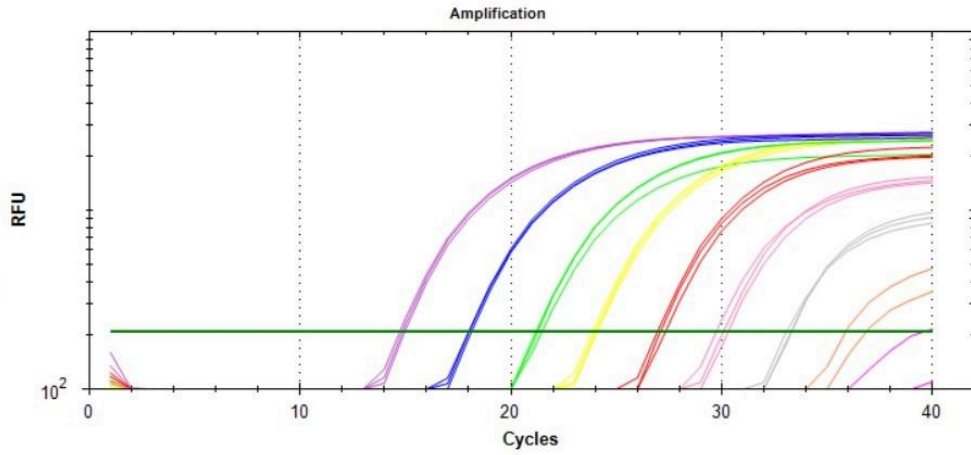

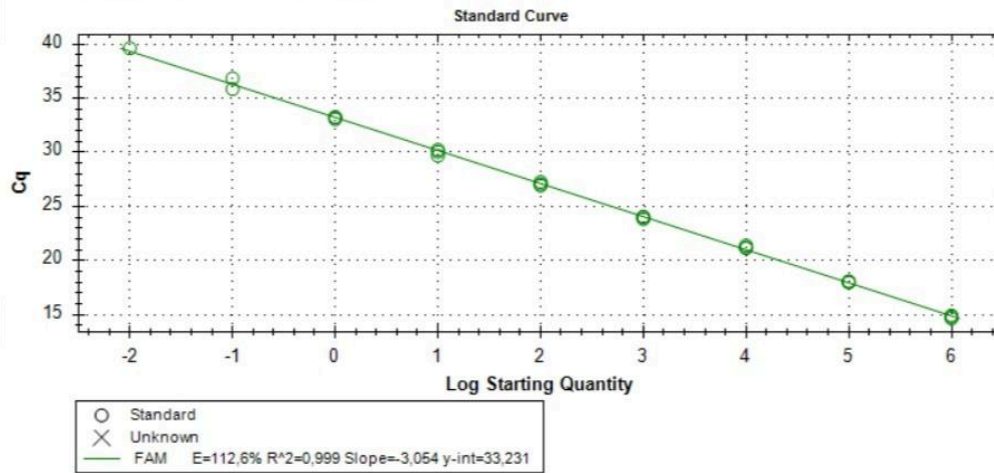

Certificate validated by:

BQ. Benjamín Catalán Soto - BQ. Rodrigo Iturra Barra  
Quality Control Managers