



Quality Control




Dilution	1	2	3	4	5	6	7	8
Concentration	1×10^{-1}	1×10^{-2}	1×10^{-3}	1×10^{-4}	1×10^{-5}	1×10^{-6}	1×10^{-7}	1×10^{-8}
Nº of copies	1×10^8	1×10^7	1×10^6	1×10^5	1×10^4	1×10^3	1×10^2	1×10^1



Target Name	Sample Name	Reporter	Ct values
<i>Actinobacillus pleuropneumoniae</i>	1	CY5	12,45
	2	CY5	14,78
	3	CY5	17,13
	4	CY5	21,43
	5	CY5	25,89
	6	CY5	28,71
	7	CY5	31,56
	8	CY5	34,98
	Negative Control	CY5	Undetermined

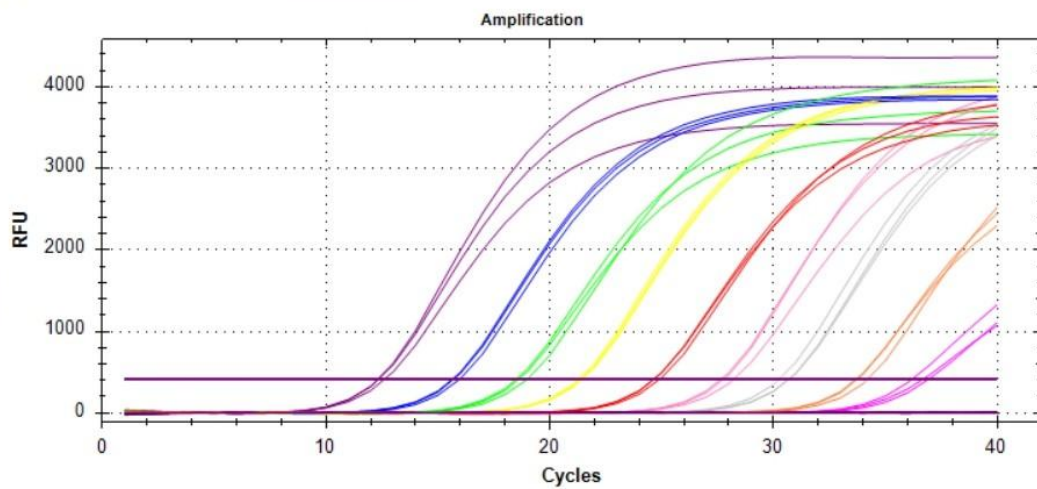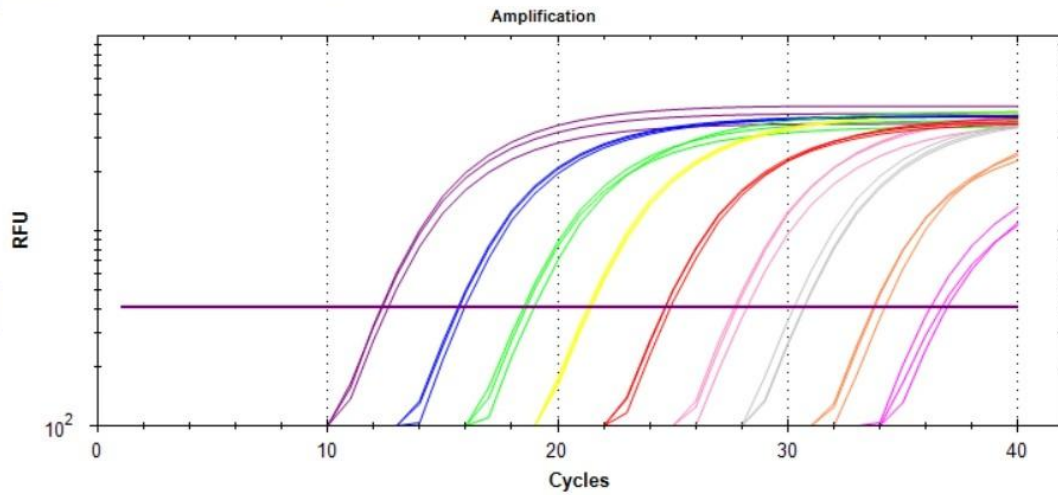

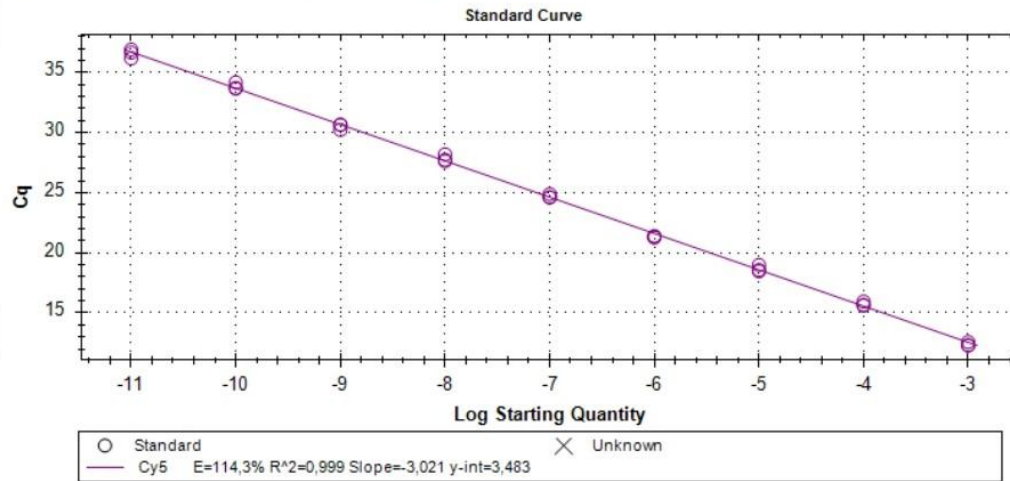

Certificate validated by:

BQ. Benjamín Catalán Soto - BQ. Rodrigo Iturra Barra

Quality Control Managers