



Quality Control




Dilution	1	2	3	4	5	6	7
Concentration	1×10^{-1}	1×10^{-2}	1×10^{-3}	1×10^{-4}	1×10^{-5}	1×10^{-6}	1×10^{-7}
N° of copies	1×10^7	1×10^6	1×10^5	1×10^4	1×10^3	1×10^2	1×10^1



Target Name	Sample Name	Reporter	Ct values
<i>Alicyclobacillus acidocaldarius</i>	1	CY5	12,32
	2	CY5	14,84
	3	CY5	17,56
	4	CY5	20,39
	5	CY5	23,92
	6	CY5	26,63
	7	CY5	30,18
	Negative Control	CY5	Undetermined

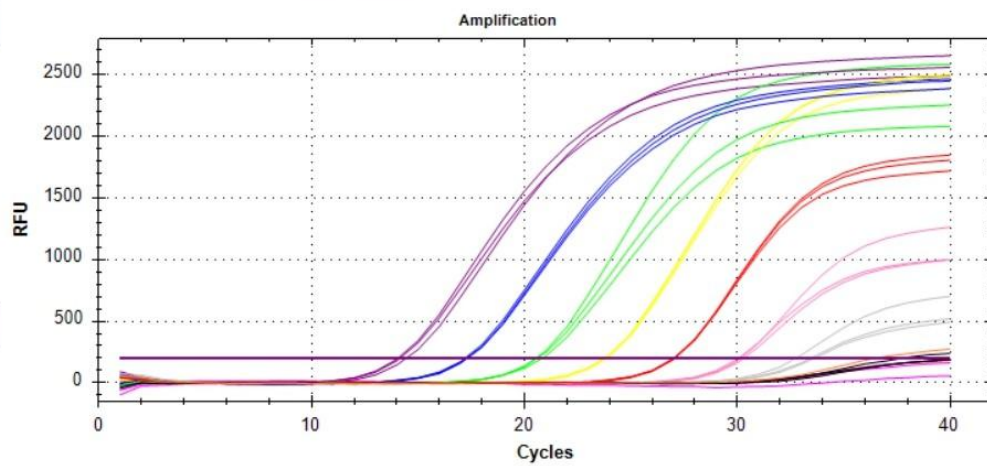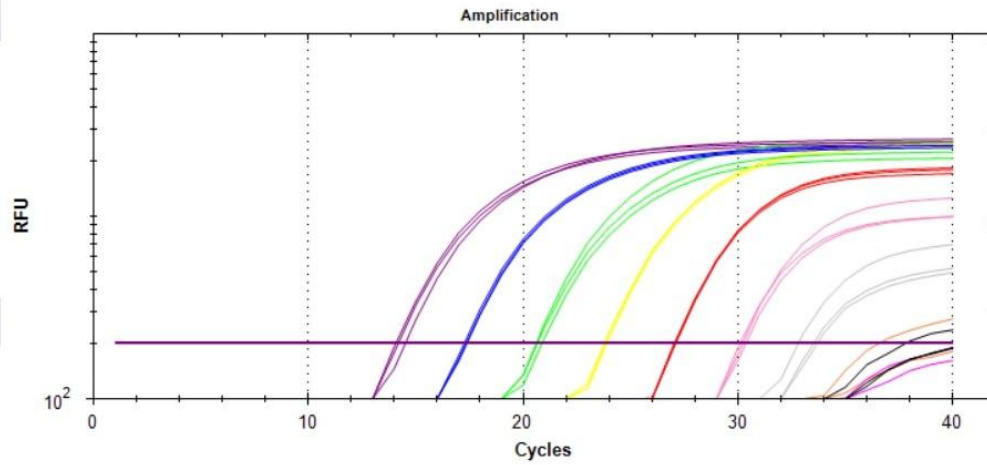

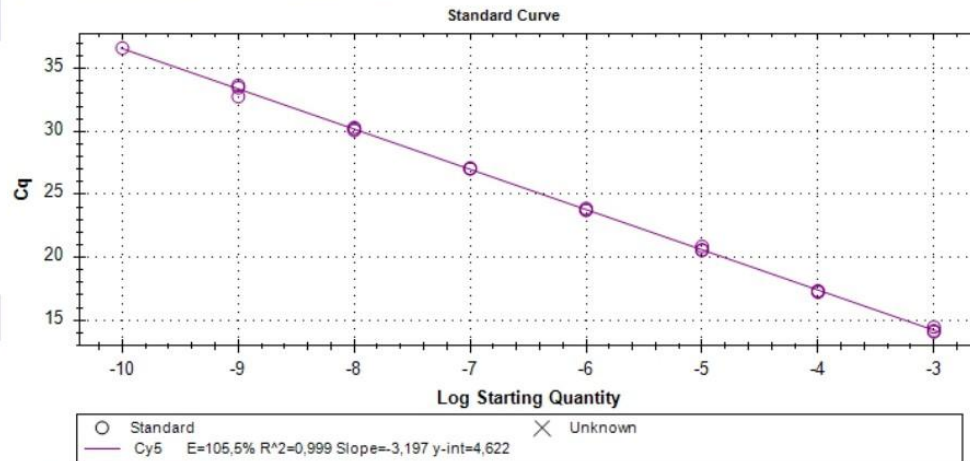

Certificate validated by:

BQ. Benjamín Catalán Soto - BQ. Rodrigo Iturra Barra
Quality Control Managers