



Quality Control




Dilution	1	2	3	4	5	6	7	8
Concentration	1×10^{-1}	1×10^{-2}	1×10^{-3}	1×10^{-4}	1×10^{-5}	1×10^{-6}	1×10^{-7}	1×10^{-8}
Nº of copies	1×10^8	1×10^7	1×10^6	1×10^5	1×10^4	1×10^3	1×10^2	1×10^1



Target Name	Sample Name	Reporter	Ct values
<i>Alicyclobacillus herbarius</i>	1	FAM	12,47
	2	FAM	14,75
	3	FAM	17,92
	4	FAM	20,57
	5	FAM	23,83
	6	FAM	26,62
	7	FAM	30,95
	8	FAM	33,26
	Negative Control	FAM	Undetermined

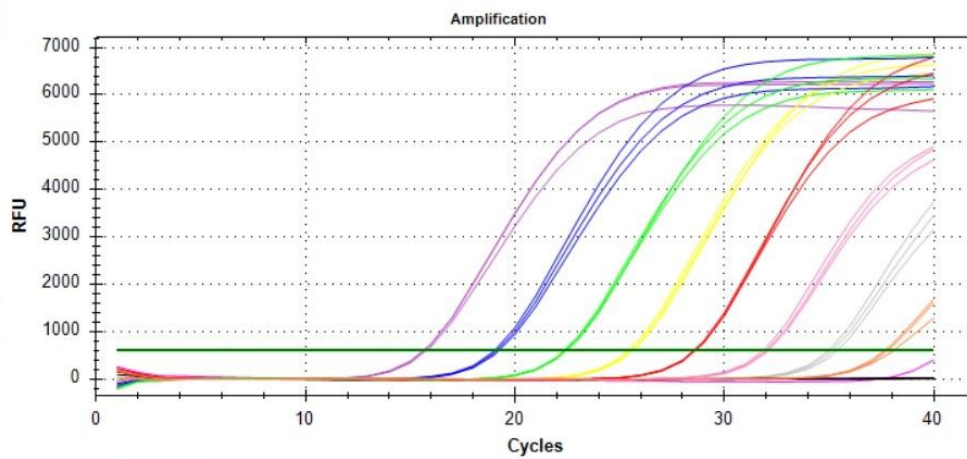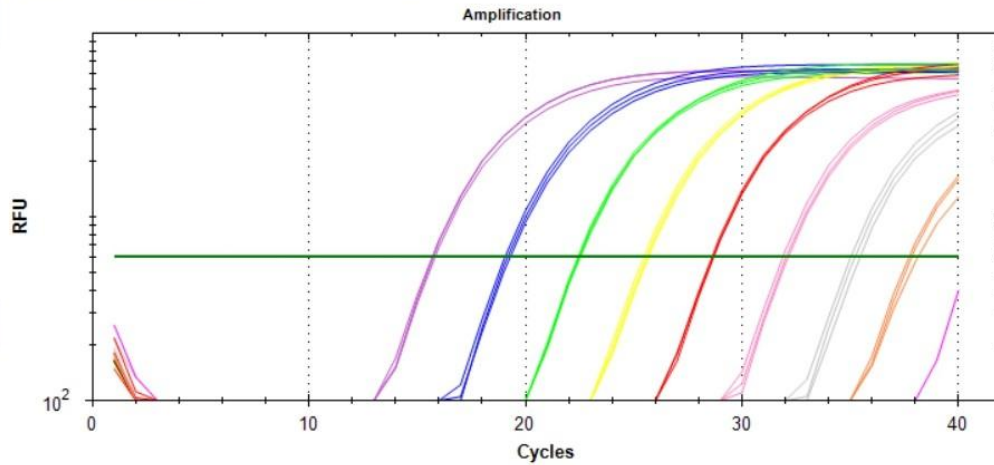

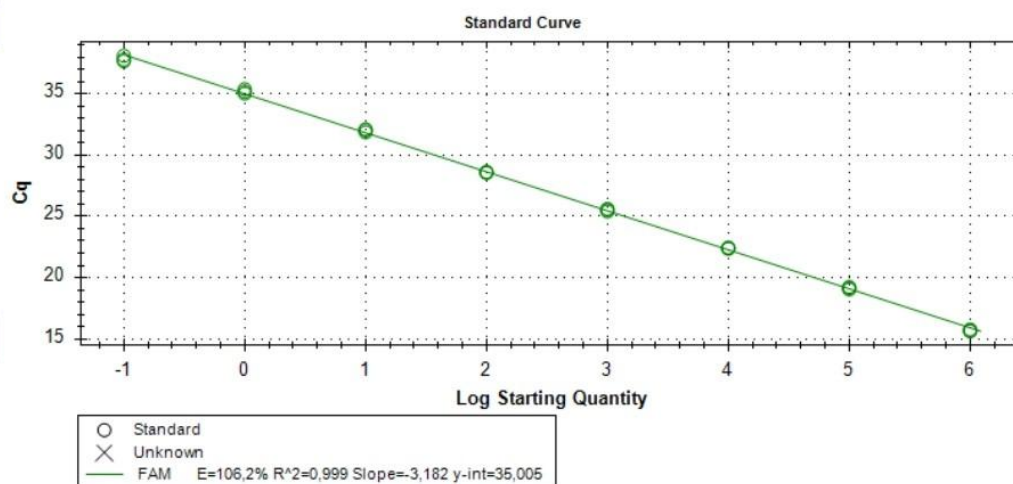

Certificate validated by:

BQ. Benjamín Catalán Soto - BQ. Rodrigo Iturra Barra

Quality Control Managers