



Quality Control




Dilution	1	2	3	4	5	6	7	8
Concentration	1×10^{-1}	1×10^{-2}	1×10^{-3}	1×10^{-4}	1×10^{-5}	1×10^{-6}	1×10^{-7}	1×10^{-8}
N° of copies	1×10^8	1×10^7	1×10^6	1×10^5	1×10^4	1×10^3	1×10^2	1×10^1



Target Name	Sample Name	Reporter	Ct values
<i>Avian infectious bronchitis</i> <i>-IB-Variant (4-91)</i>	1	FAM	11,56
	2	FAM	15,47
	3	FAM	18,38
	4	FAM	21,85
	5	FAM	25,57
	6	FAM	28,48
	7	FAM	31,38
	8	FAM	34,74
	Negative Control	FAM	Undetermined

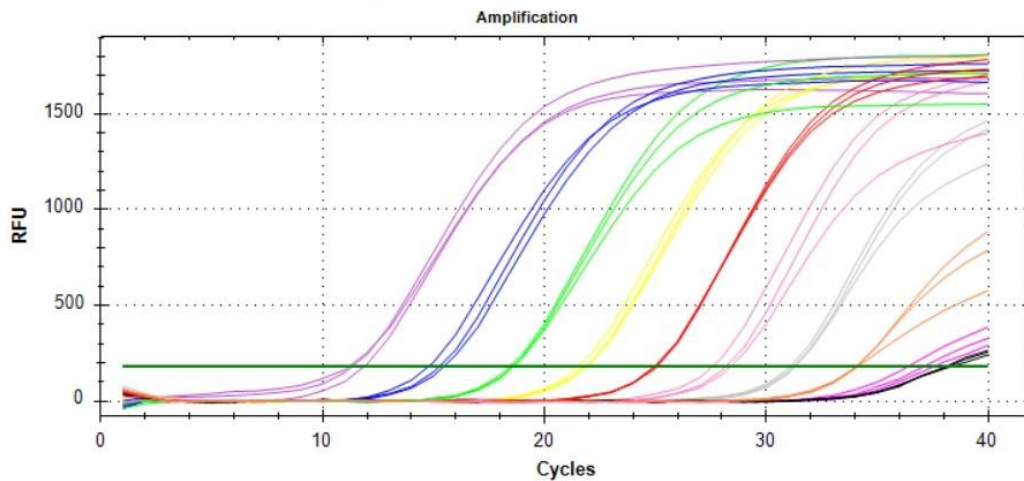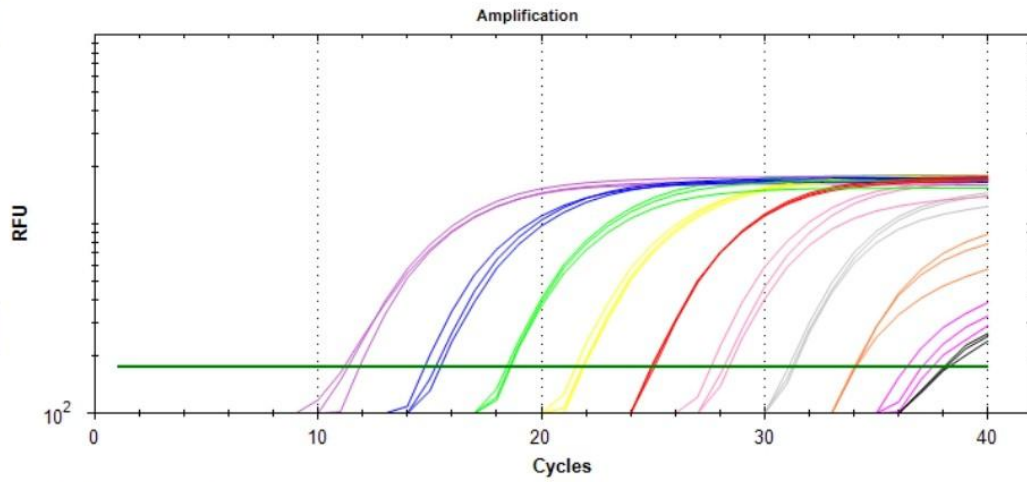

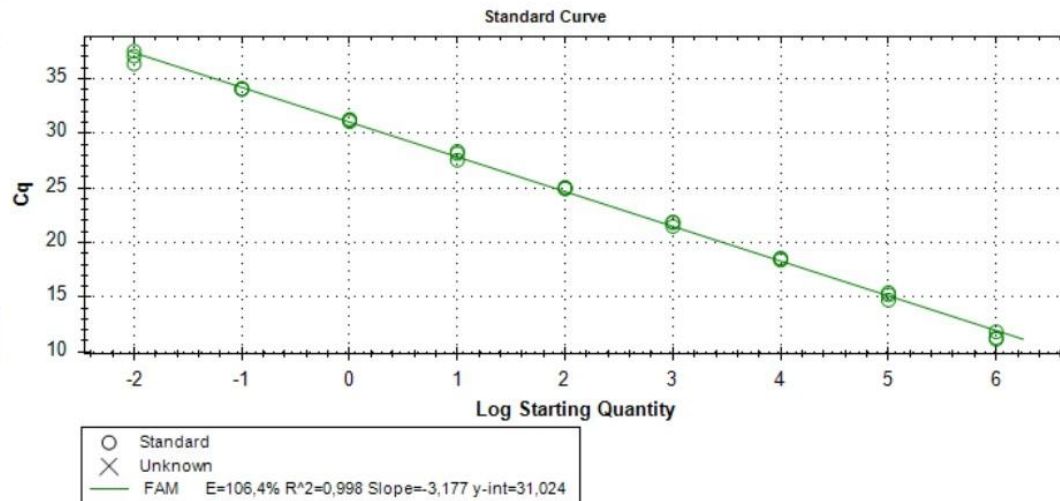

Certificate validated by:

BQ. Benjamín Catalán Soto - BQ. Rodrigo Iturra Barra

Quality Control Managers