



Quality Control




Dilution	1	2	3	4	5	6	7	8
Concentration	1×10^{-1}	1×10^{-2}	1×10^{-3}	1×10^{-4}	1×10^{-5}	1×10^{-6}	1×10^{-7}	1×10^{-8}
N° of copies	1×10^8	1×10^7	1×10^6	1×10^5	1×10^4	1×10^3	1×10^2	1×10^1



Target Name	Sample Name	Reporter	Ct values
<i>Avian infectious bronchitis virus</i> <i>Variant Israel 02</i>	1	FAM	14,34
	2	FAM	17,75
	3	FAM	20,35
	4	FAM	23,86
	5	FAM	27,45
	6	FAM	31,26
	7	FAM	34,74
	8	FAM	37,25
	Negative Control	FAM	Undetermined

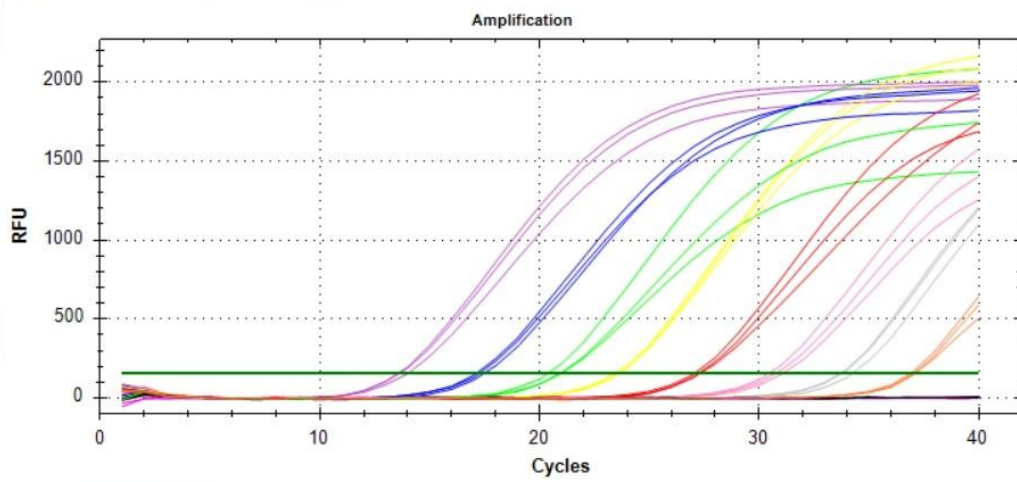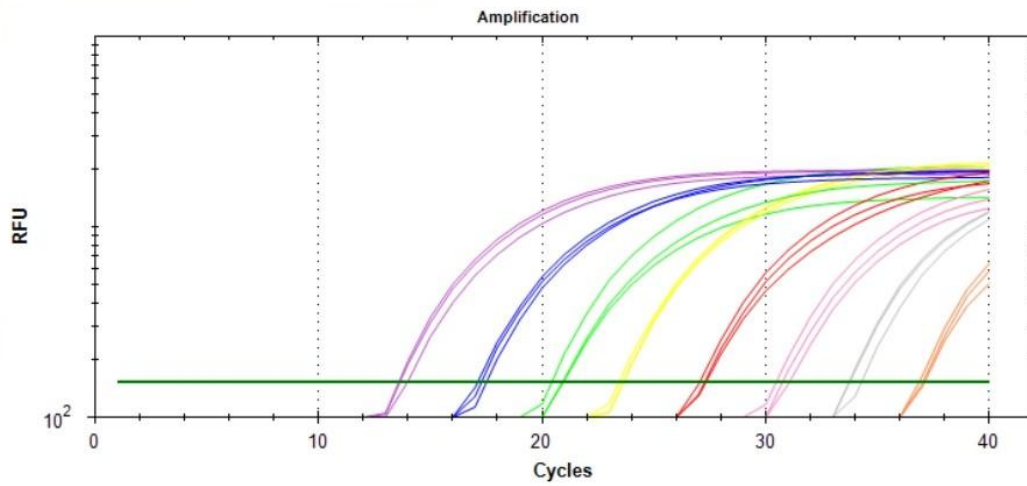

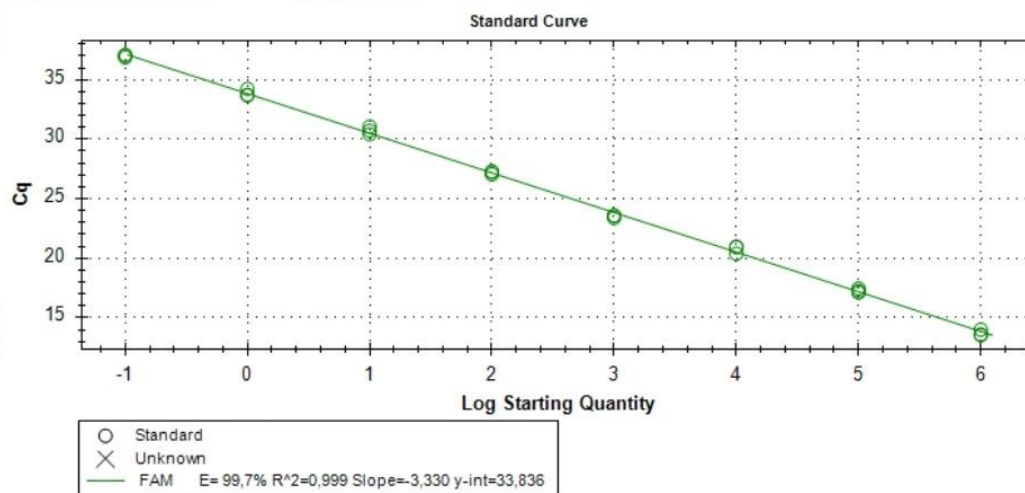

Certificate validated by:

BQ. Benjamín Catalán Soto - BQ. Rodrigo Iturra Barra

Quality Control Managers