



Quality Control




Dilution	1	2	3	4	5	6	7
Concentration	1×10^{-1}	1×10^{-2}	1×10^{-3}	1×10^{-4}	1×10^{-5}	1×10^{-6}	1×10^{-7}
N° of copies	1×10^7	1×10^6	1×10^5	1×10^4	1×10^3	1×10^2	1×10^1



Target Name	Sample Name	Reporter	Ct values
<i>Avian metapneumovirus – Subtypes A&B</i>	1	ROX	12,32
	2	ROX	15,65
	3	ROX	19,48
	4	ROX	23,95
	5	ROX	26,63
	6	ROX	30,65
	7	ROX	33,97
	Negative Control	ROX	Undetermined

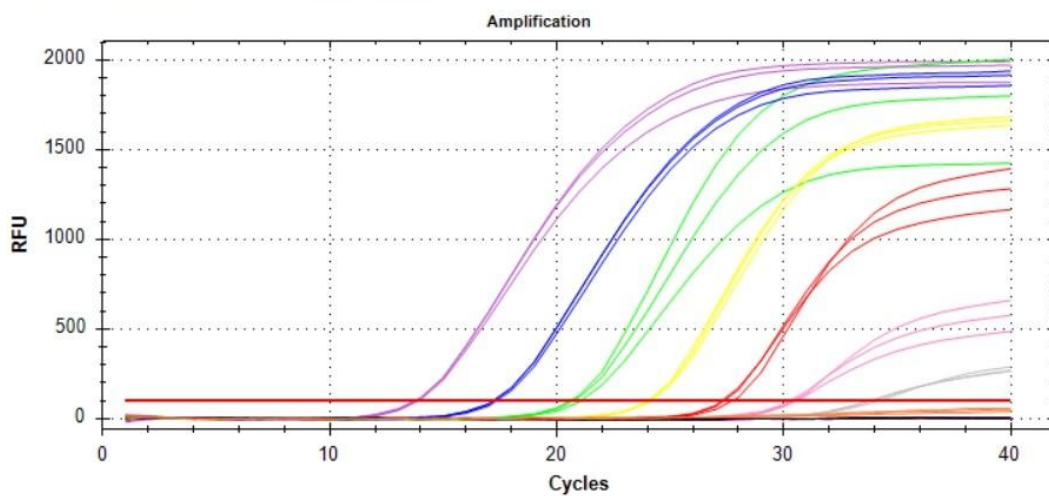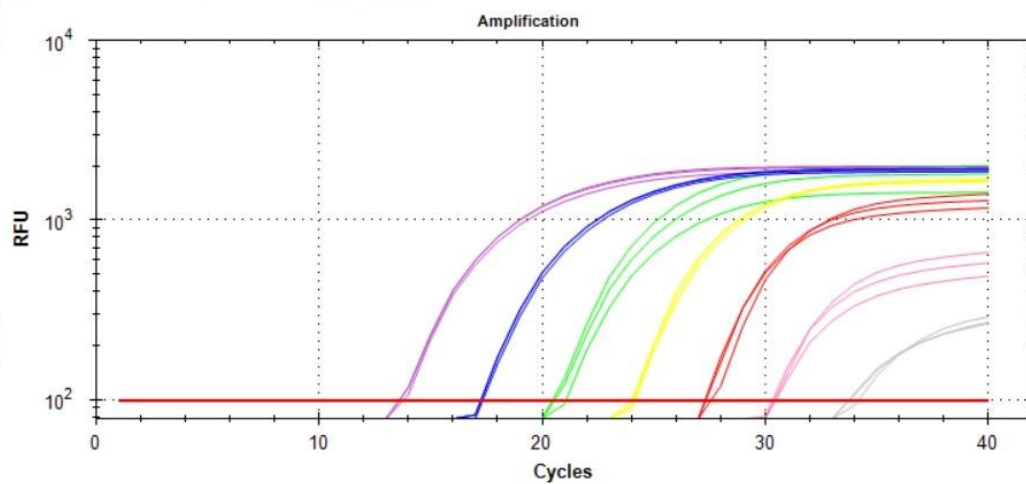

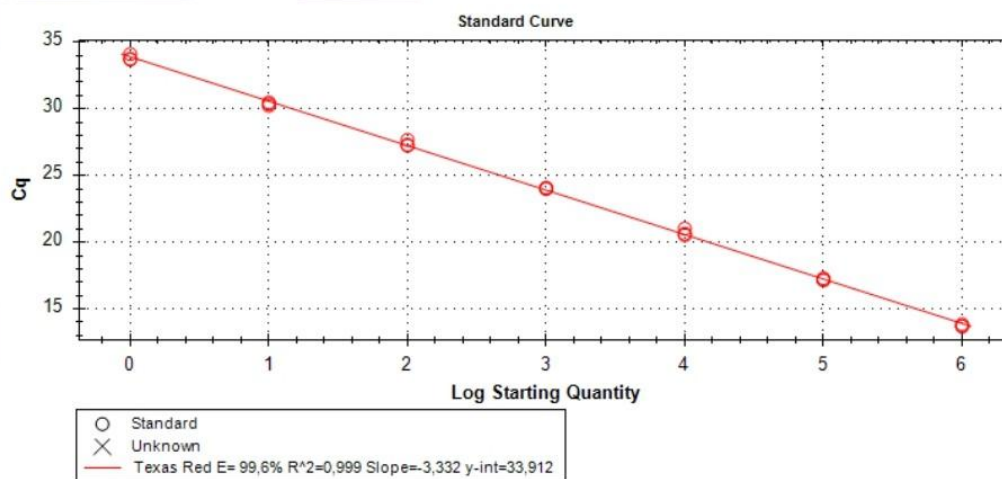

Certificate validated by:

BQ. Benjamín Catalán Soto - BQ. Rodrigo Iturra Barra

Quality Control Managers