



Quality Control




Dilution	1	2	3	4	5	6	7	8
Concentration	1×10^{-1}	1×10^{-2}	1×10^{-3}	1×10^{-4}	1×10^{-5}	1×10^{-6}	1×10^{-7}	1×10^{-8}
N° of copies	1×10^8	1×10^7	1×10^6	1×10^5	1×10^4	1×10^3	1×10^2	1×10^1



Target Name	Sample Name	Reporter	Ct values
<i>Bordetella bronchiseptica</i>	1	CY5	13,37
	2	CY5	17,04
	3	CY5	22,85
	4	CY5	25,34
	5	CY5	27,76
	6	CY5	30,68
	7	CY5	32,74
	8	CY5	35,93
	Negative Control	CY5	Undetermined

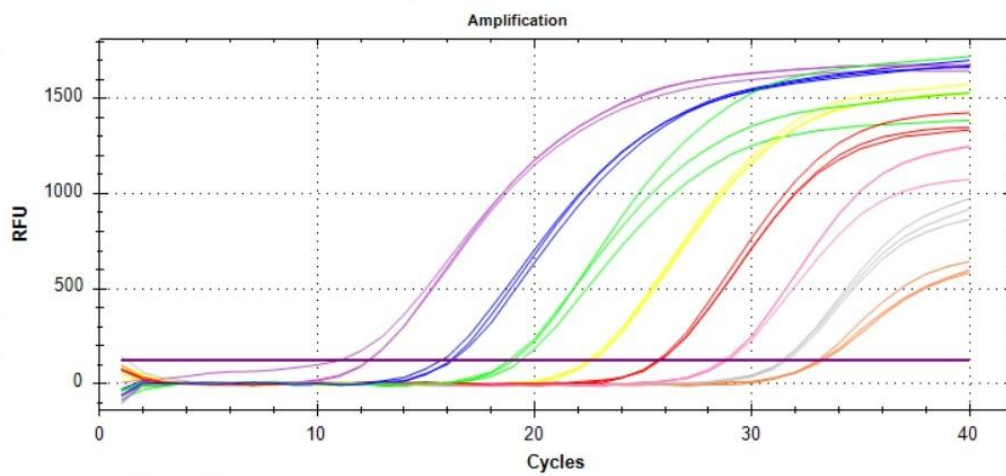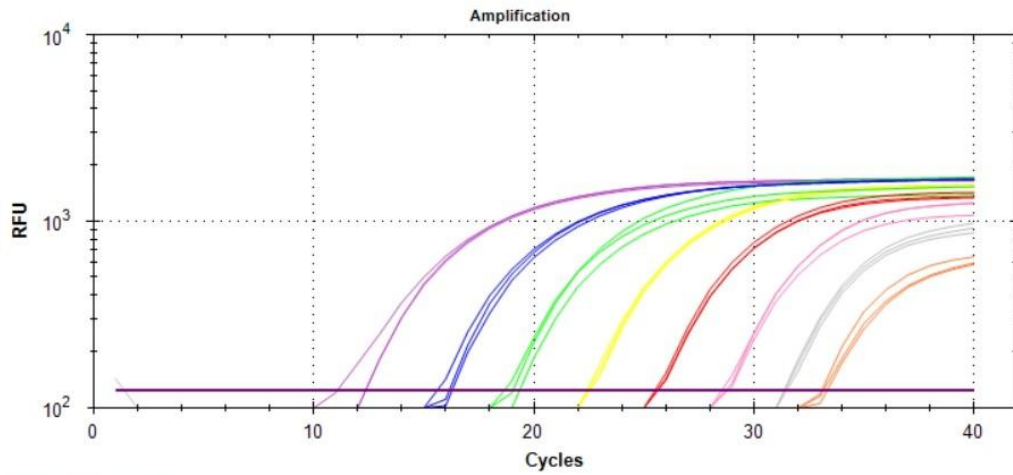

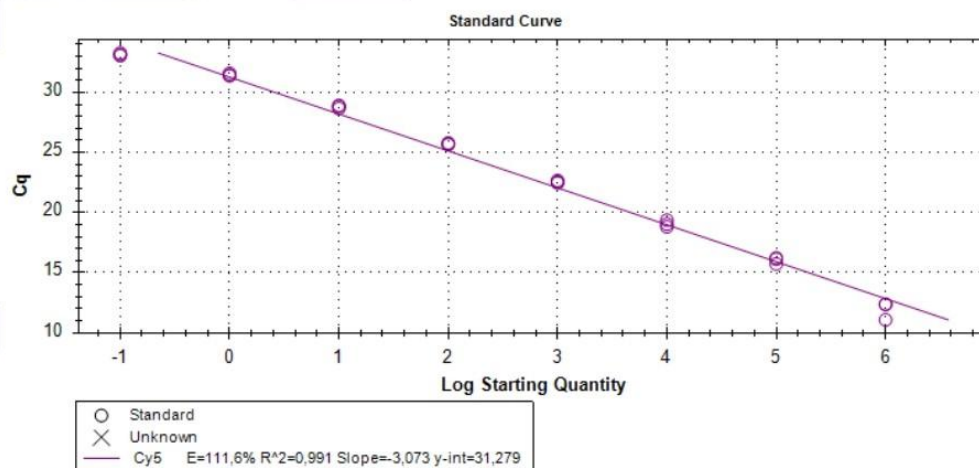

Certificate validated by:

BQ. Benjamín Catalán Soto - BQ. Rodrigo Iturra Barra
 Quality Control Managers