BioinGentech
Biotechnology

PCR Kit Quality Control Certificate

Pathogen
Chlamydophila spp.

Table 1: Concentration in ng/µL of the sample control and its dilutions.

	1	2	3	4	5	6	7	8
	$1x10^{-1}$	$1x10^{-2}$	$1x10^{-3}$	$1x10^{-4}$	$1x10^{-5}$	$1x10^{-6}$	$1x10^{-7}$	$1x10^{-8}$
N° of copies	$1x10^{8}$	$1x10^{7}$	$1x10^{6}$	$1x10^{5}$	$1x10^{4}$	$1x10^{3}$	$1x10^{2}$	$1x10^{1}$

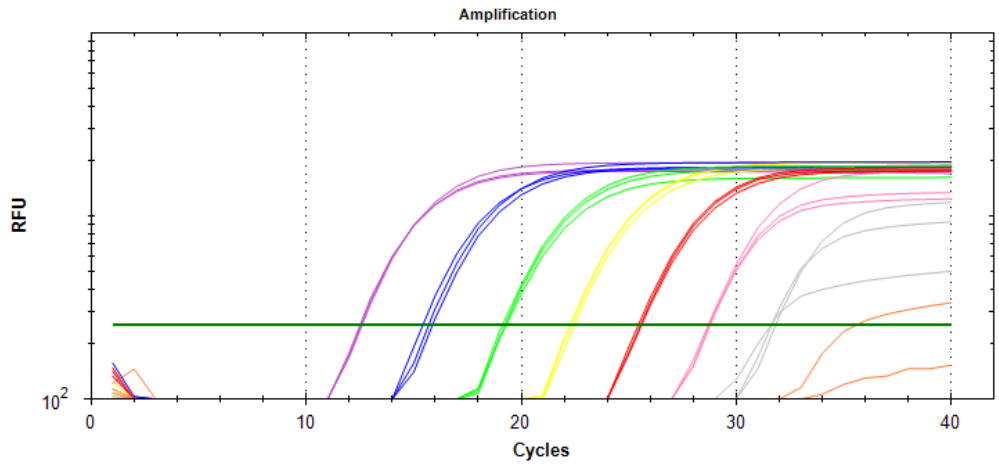

Figure 1: Logarithmic amplification curves for Chlamydophila spp.

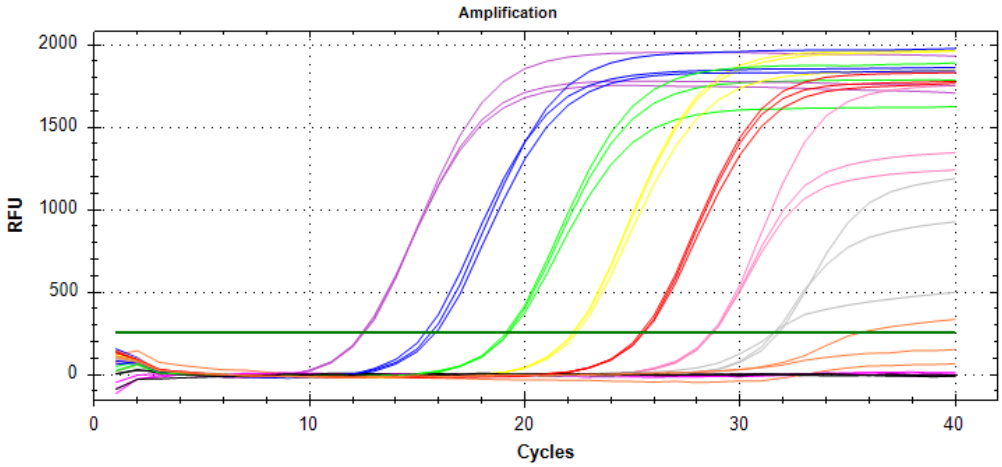

Figure 2: Standard amplification curves for Chlamydophila spp.

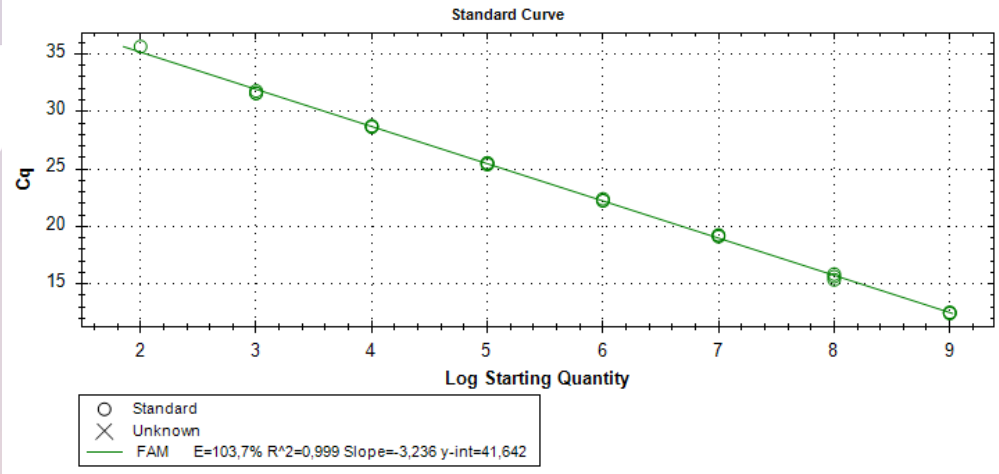

Figure 3: Standard curve for Chlamydophila spp.

Summary of Ct values

Table 2: Ct values obtained for each dilution of the sample control.

Target Name	Sample Name	Reporter	Ct values
Chlamydophila spp.	1	FAM	12,43
	2	FAM	15,36
	3	FAM	19,11
	4	FAM	22,25
	5	FAM	25,53
	6	FAM	28,71
	7	FAM	31,59
	8	FAM	35,65
	Negative Control	FAM	Undetermined

Certificate validated by:

BQ. Benjamín Catalan - BQ. Rodrigo Iturra Barra

Quality Control Managers