


# PCR Kit Quality Control Certificate


Pathogen
<i>Clavibacter michiganensis subsp. sepedonicus</i>

**Table 1: Concentration in ng/ $\mu$ L of the sample control and its dilutions.**


	1	2	3	4	5	6	7	8
	$1 \times 10^{-1}$	$1 \times 10^{-2}$	$1 \times 10^{-3}$	$1 \times 10^{-4}$	$1 \times 10^{-5}$	$1 \times 10^{-6}$	$1 \times 10^{-7}$	$1 \times 10^{-8}$
N° of copies	$1 \times 10^8$	$1 \times 10^7$	$1 \times 10^6$	$1 \times 10^5$	$1 \times 10^4$	$1 \times 10^3$	$1 \times 10^2$	$1 \times 10^1$

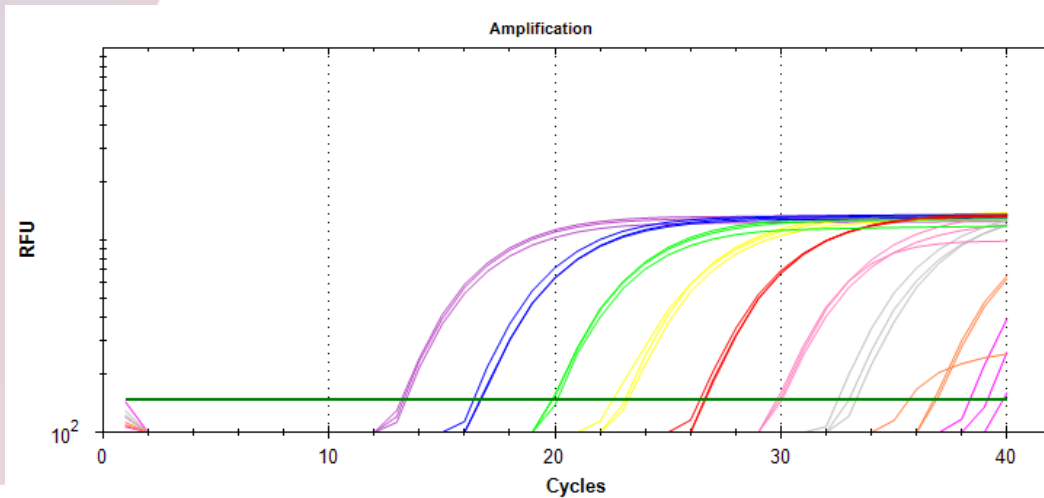

**Figure 1: Logarithmic amplification curves for *Clavibacter michiganensis subsp. sepedonicus***

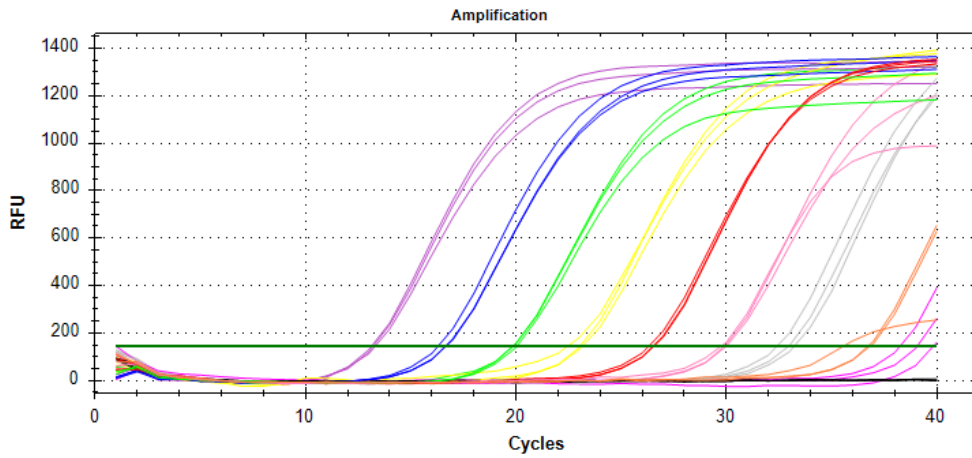

**Figure 2: Standard amplification curves for *Clavibacter michiganensis subsp. sepedonicus***

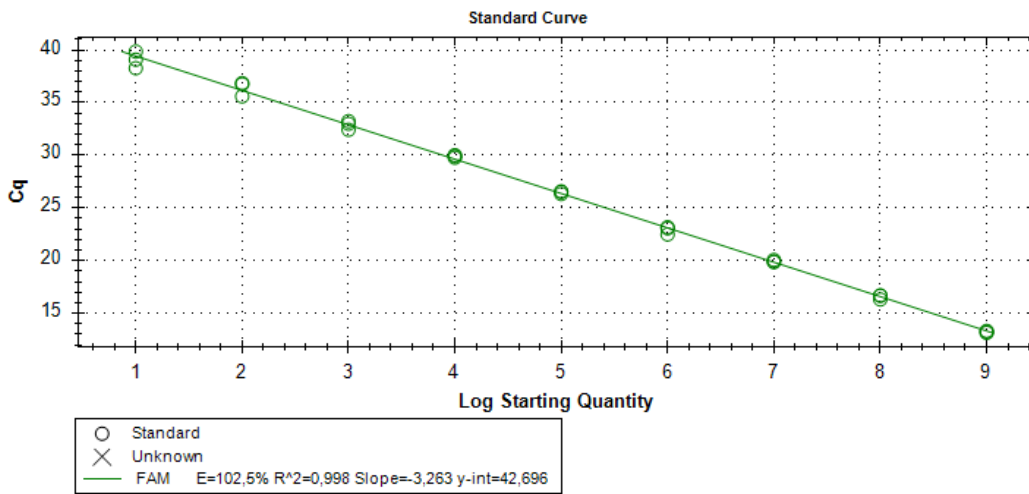

**Figure 3: Standard curve for *Clavibacter michiganensis subsp. sepedonicus***

## Summary of Ct values

**Table 2:** Ct values obtained for each dilution of the sample control.

Target Name	Sample Name	Reporter	Ct values
<i>Clavibacter michiganensis subsp. sepedonicus</i>	1	FAM	13,33
	2	FAM	16,32
	3	FAM	19,87
	4	FAM	23,06
	5	FAM	26,33
	6	FAM	29,78
	7	FAM	33
	8	FAM	36,86
	Negative Control	FAM	Undetermined

Certificate validated by:

**BQ. Benjamín Catalán - BQ. Rodrigo Iturra Barra**  
**Quality Control Managers**