



Quality Control




Dilution	1	2	3	4	5	6	7	8
Concentration	1×10^{-1}	1×10^{-2}	1×10^{-3}	1×10^{-4}	1×10^{-5}	1×10^{-6}	1×10^{-7}	1×10^{-8}
Nº of copies	1×10^8	1×10^7	1×10^6	1×10^5	1×10^4	1×10^3	1×10^2	1×10^1



Target Name	Sample Name	Reporter	Ct values
<i>Edwardsiella tarda</i>	1	FAM	12,73
	2	FAM	15,63
	3	FAM	19,27
	4	FAM	23,46
	5	FAM	26,27
	6	FAM	30,84
	7	FAM	33,63
	8	FAM	36,27
	Negative Control	FAM	Undetermined

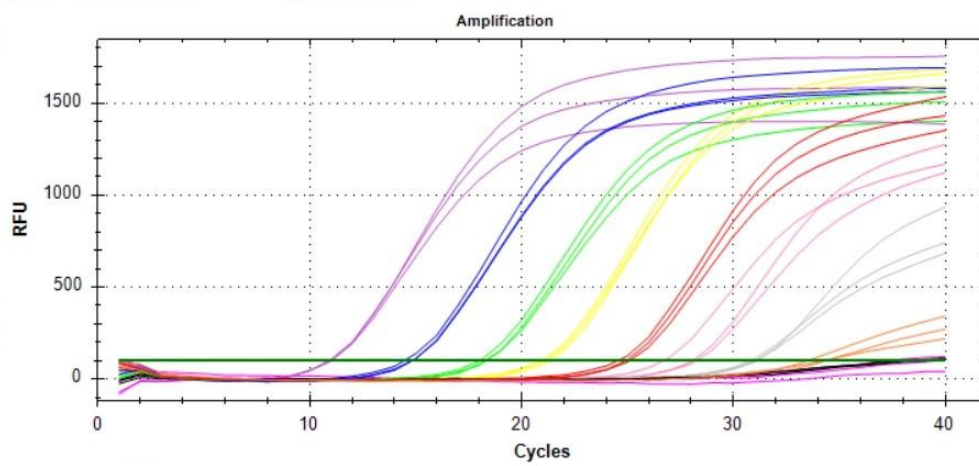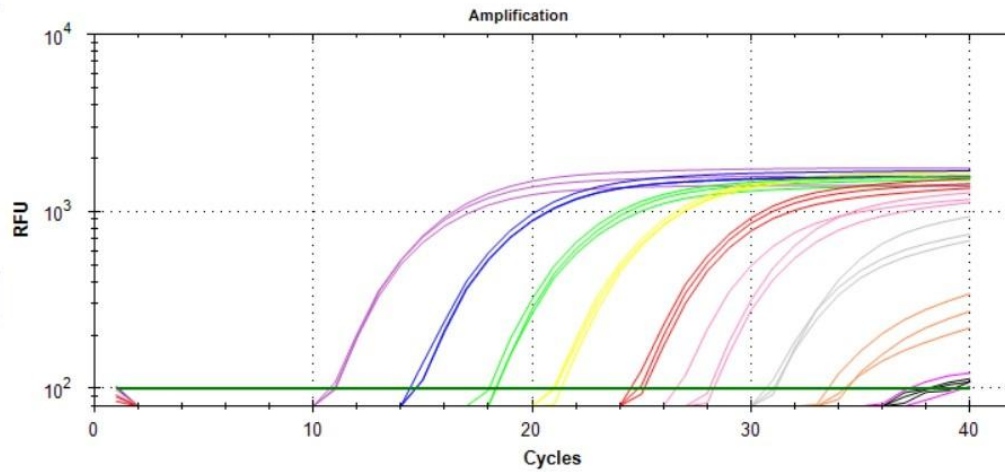

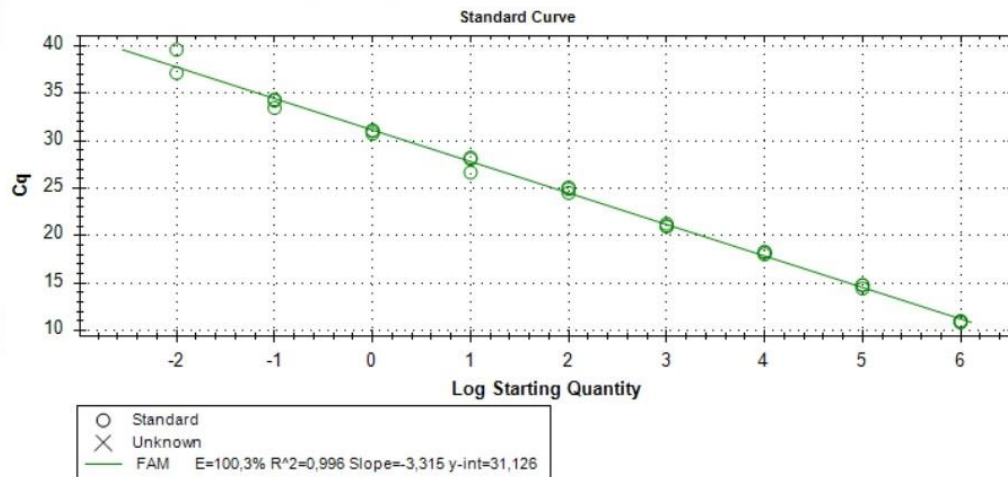

Certificate validated by:

BQ. Benjamín Catalán Soto - BQ. Rodrigo Iturra Barra

Quality Control Managers