



Quality Control




Dilution	1	2	3	4	5	6	7	8
Concentration	1×10^{-1}	1×10^{-2}	1×10^{-3}	1×10^{-4}	1×10^{-5}	1×10^{-6}	1×10^{-7}	1×10^{-8}
Nº of copies	1×10^8	1×10^7	1×10^6	1×10^5	1×10^4	1×10^3	1×10^2	1×10^1



Target Name	Sample Name	Reporter	Ct values
<i>Foot-and-Mouth Disease Virus (FMDV) SAT2</i>	1	ROX	13,41
	2	ROX	16,48
	3	ROX	19,67
	4	ROX	22,88
	5	ROX	26,11
	6	ROX	29,55
	7	ROX	32,61
	8	ROX	36,68
	Negative Control	ROX	Undetermined

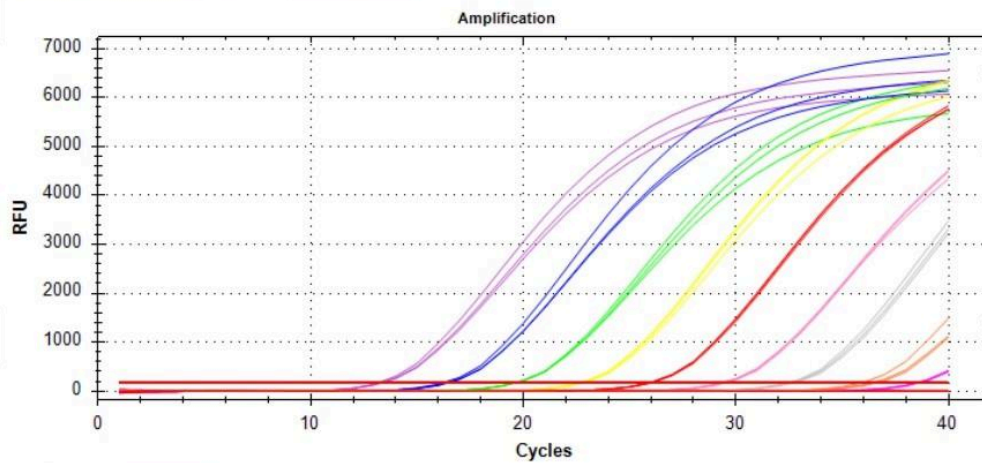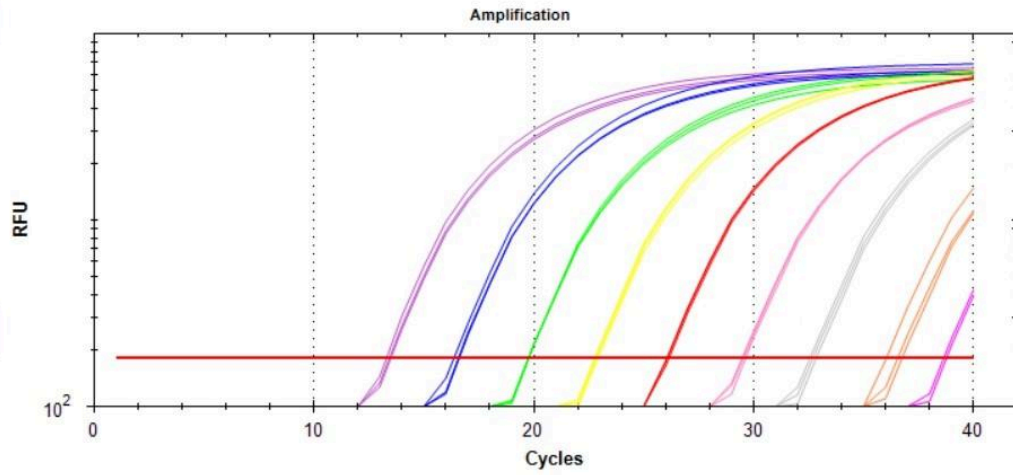

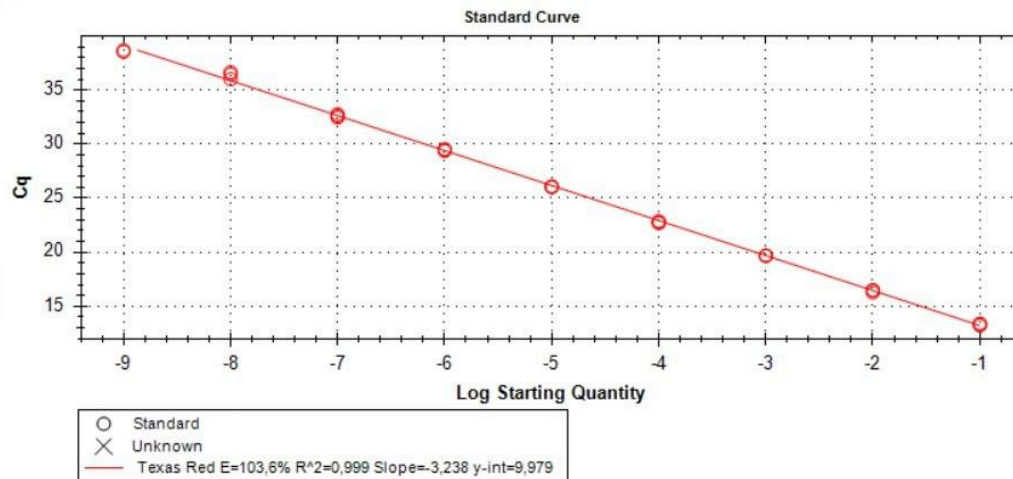

Certificate validated by:

BQ. Benjamín Catalán Soto - BQ. Rodrigo Iturra Barra

Quality Control Managers