

PCR Kit Quality Control Certificate

Pathogen
<i>Salmonella Enteriditis</i>

Table 1: Concentration in ng/μL of the sample control and its dilutions.

	1	2	3	4	5	6	7	8
	1×10^{-1}	1×10^{-2}	1×10^{-3}	1×10^{-4}	1×10^{-5}	1×10^{-6}	1×10^{-7}	1×10^{-8}
N° of copies	1×10^8	1×10^7	1×10^6	1×10^5	1×10^4	1×10^3	1×10^2	1×10^1

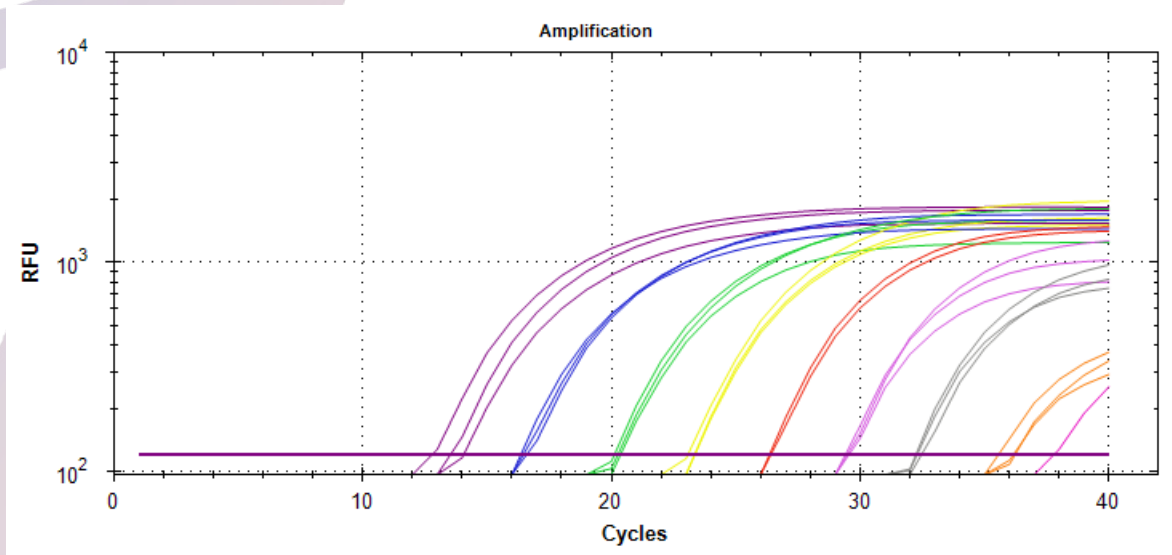


Figure 1: Logarithmic amplification curves for *Salmonella Enteriditis*

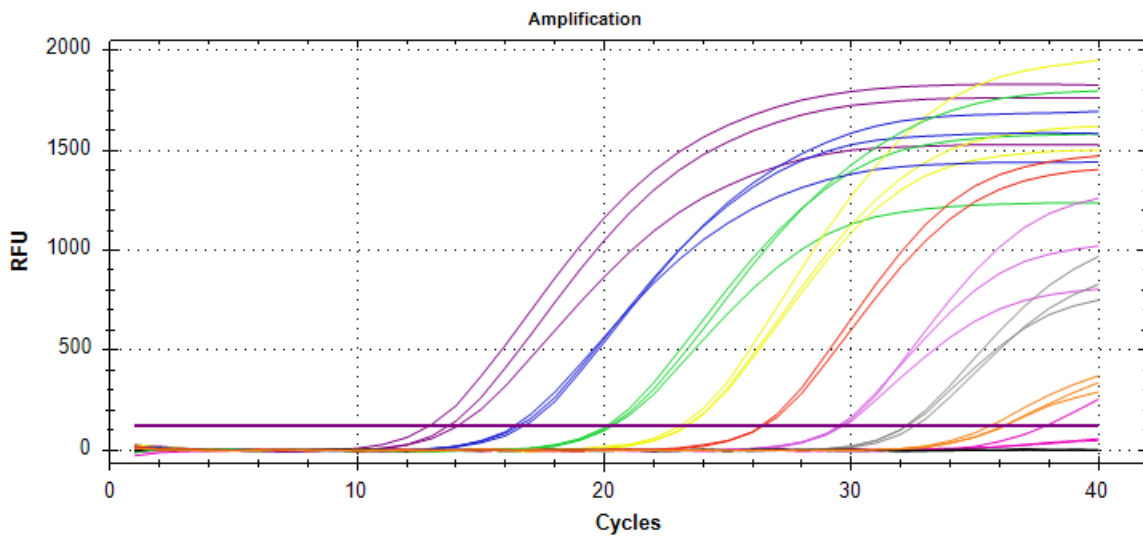


Figure 2: Standard amplification curves for *Salmonella Enteritidis*

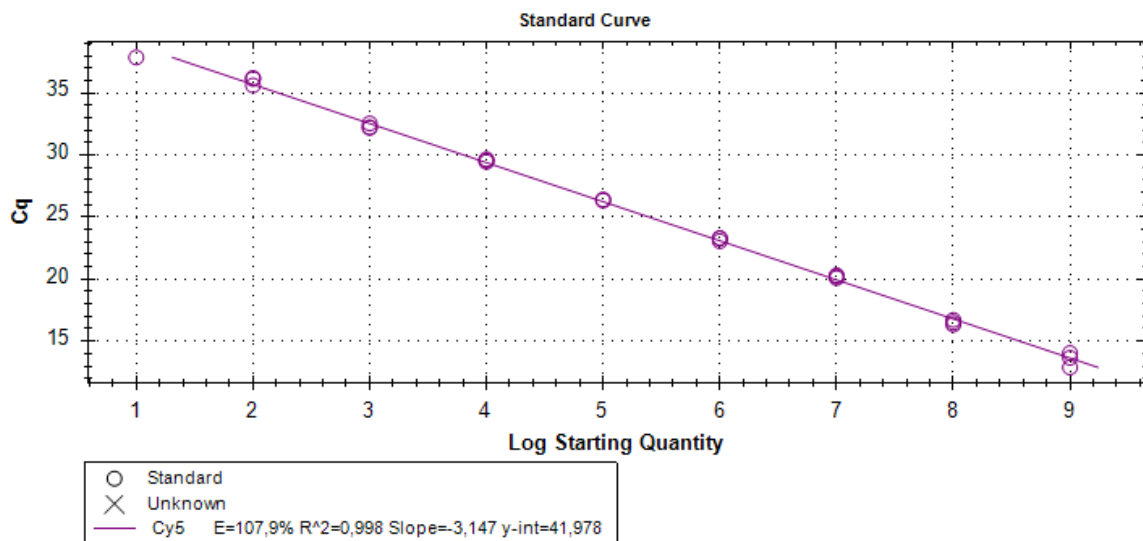


Figure 3: Standard curve for *Salmonella Enteritidis*

Pathogen

Salmonella Typhimurium

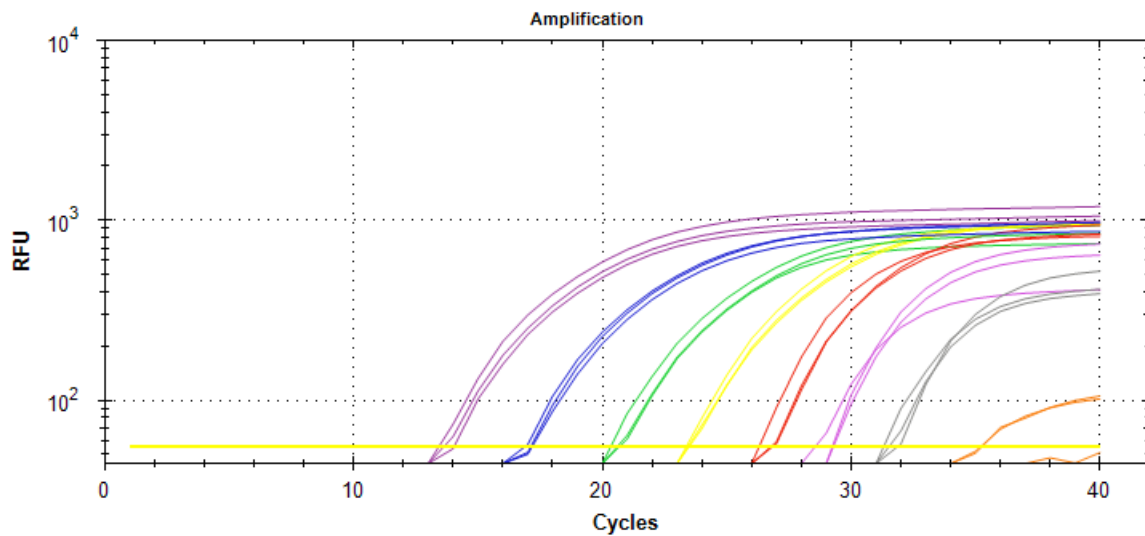


Figure 4: Logarithmic amplification curves for *Salmonella Typhimurium*

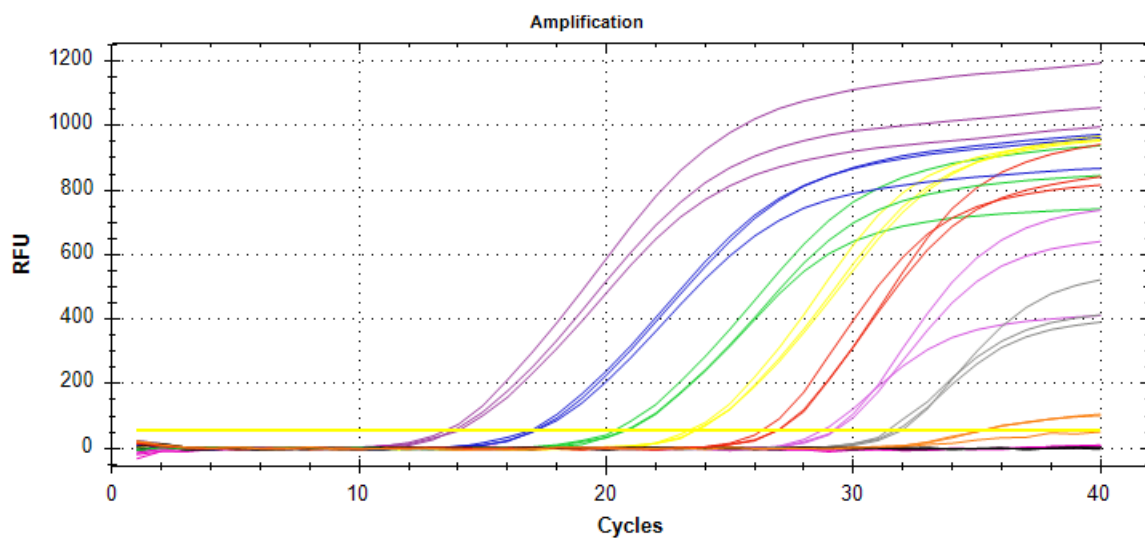


Figure 5: Standard amplification curves for *Salmonella Typhimurium*

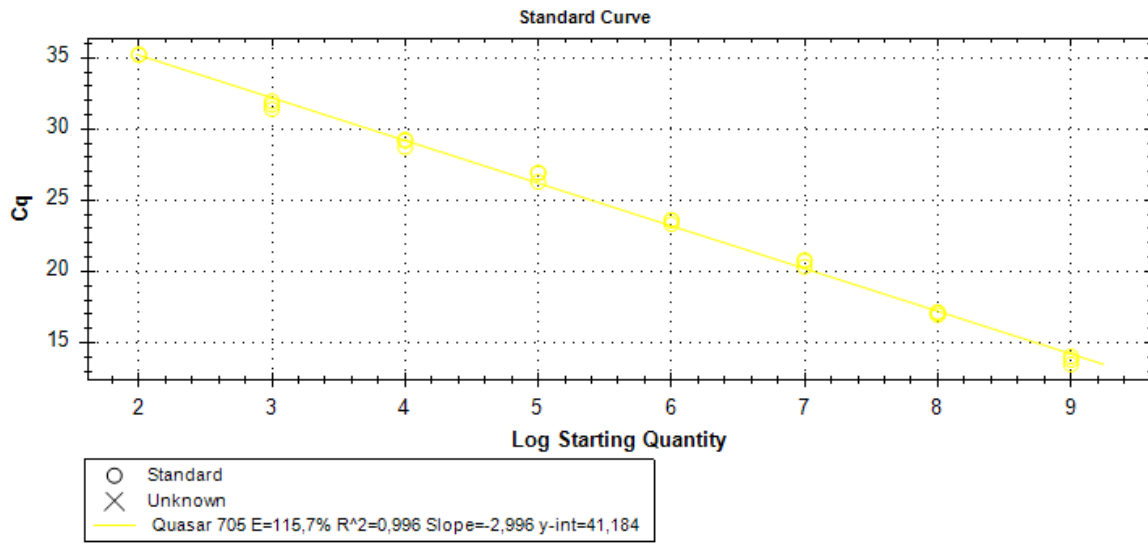


Figure 6: Standard curve for *Salmonella Typhimurium*

Summary of Ct values

Table 2: Ct values obtained for each dilution of the sample control.

Target Name	Sample Name	Reporter	Ct values
<i>Salmonella Enteriditis</i>	1	CY5	12,15
	2	CY5	15,79
	3	CY5	18,41
	4	CY5	22,17
	5	CY5	25,38
	6	CY5	28,01
	7	CY5	31,92
	8	CY5	-
	Negative Control	CY5	Undetermined

Target Name	Sample Name	Reporter	Ct values
<i>Salmonella Typhimurium</i>	1	CY5.5	14,04
	2	CY5.5	16,95
	3	CY5.5	20,72
	4	CY5.5	23,61
	5	CY5.5	26,91
	6	CY5.5	28,74
	7	CY5.5	31,96
	8	CY5.5	35,21
	Negative Control	CY5.5	Undetermined

Certificate validated by:

BQ. Benjamín Catalan - BQ. Rodrigo Iturra Barra

Quality Control Managers