


# PCR Kit Quality Control Certificate


Pathogen
<i>Mycosphaerella fragariae</i>

**Table 1: Concentration in ng/μL of the sample control and its dilutions.**


	1	2	3	4	5	6	7	8	9
	$1 \times 10^{-1}$	$1 \times 10^{-2}$	$1 \times 10^{-3}$	$1 \times 10^{-4}$	$1 \times 10^{-5}$	$1 \times 10^{-6}$	$1 \times 10^{-7}$	$1 \times 10^{-8}$	$1 \times 10^{-9}$
N° of copies	$1 \times 10^8$	$1 \times 10^7$	$1 \times 10^6$	$1 \times 10^5$	$1 \times 10^4$	$1 \times 10^3$	$1 \times 10^2$	$1 \times 10^1$	$1 \times 10^0$

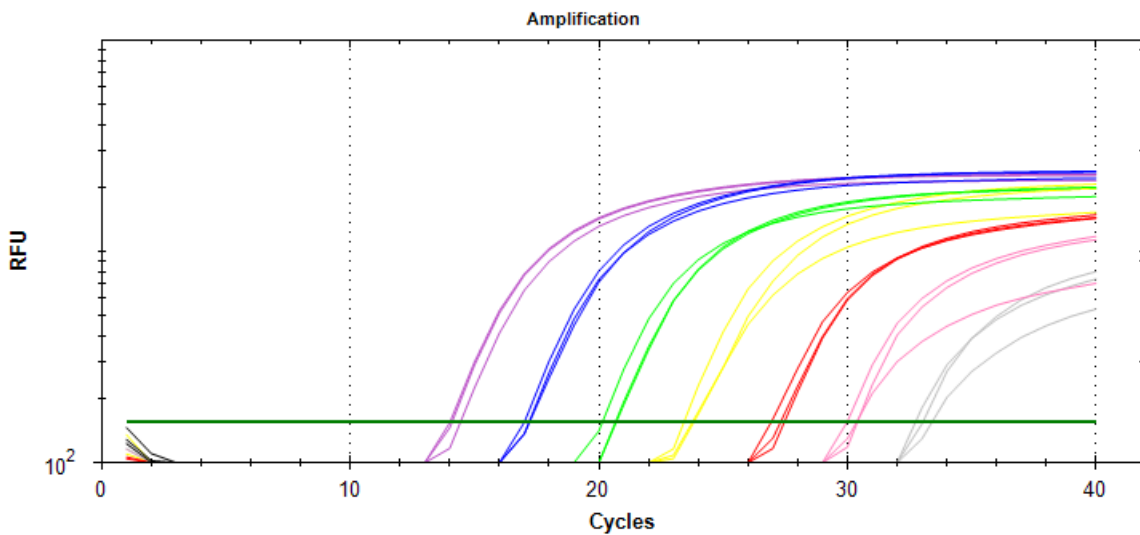

**Figure 1: Logarithmic amplification curves for *Mycosphaerella fragariae***

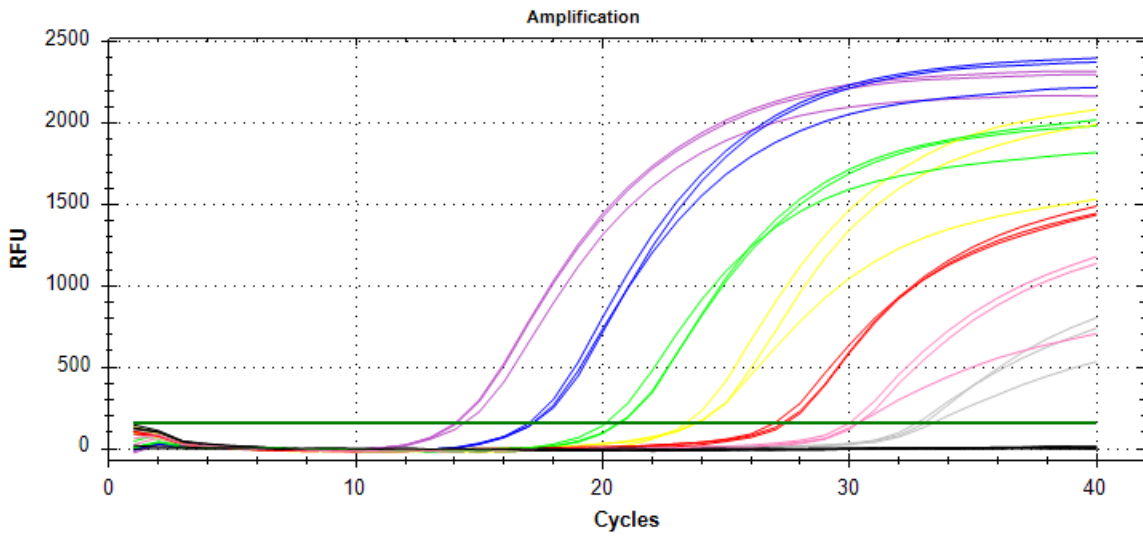

*Figure 2: Standard amplification curves for Mycosphaerella fragariae*

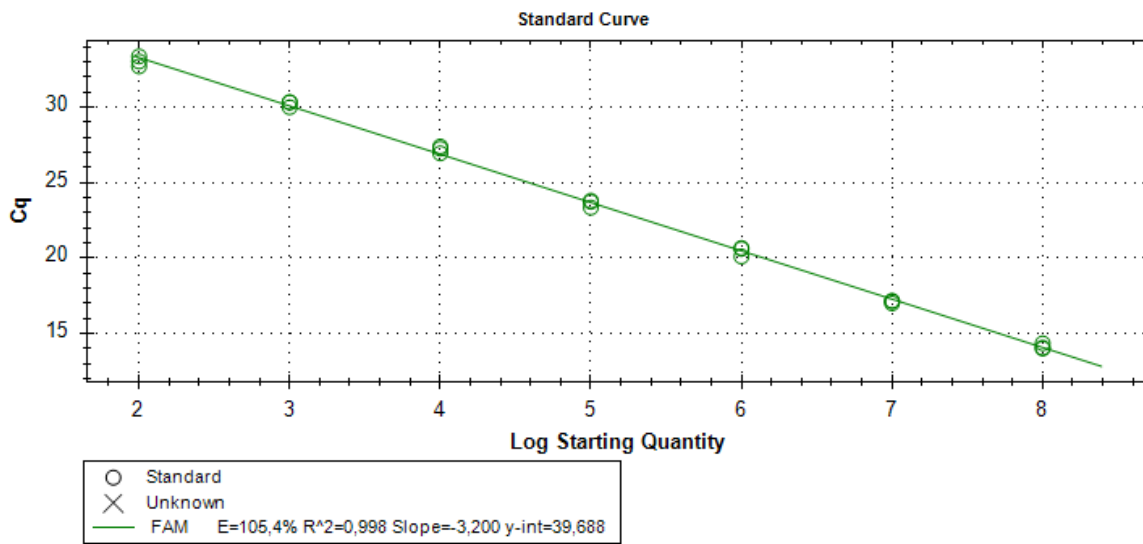

*Figure 3: Standard curve for Mycosphaerella fragariae*

## Summary of Ct values

**Table 2:** Ct values obtained for each dilution of the sample control.

Target Name	Sample Name	Reporter	Ct values
<i>Mycosphaerella fragariae</i>	1	FAM	14,32
	2	FAM	17,12
	3	FAM	20,63
	4	FAM	23,71
	5	FAM	27,23
	6	FAM	30,33
	7	FAM	32,67
	Negative Control	FAM	Undetermined