BioinGentech
Biotechnology

PCR Kit Quality Control Certificate

Pathogen
Prunus Necrotic Ringspot Virus

Table 1: Concentration in ng/µL of the sample control and its dilutions.

	1	2	3	4	5	6	7	8
	$1x10^{-1}$	$1x10^{-2}$	$1x10^{-3}$	$1x10^{-4}$	$1x10^{-5}$	$1x10^{-6}$	$1x10^{-7}$	$1x10^{-8}$
N° of copies	$1x10^{8}$	$1x10^{7}$	$1x10^{6}$	$1x10^{5}$	$1x10^{4}$	$1x10^{3}$	$1x10^{2}$	$1x10^{1}$

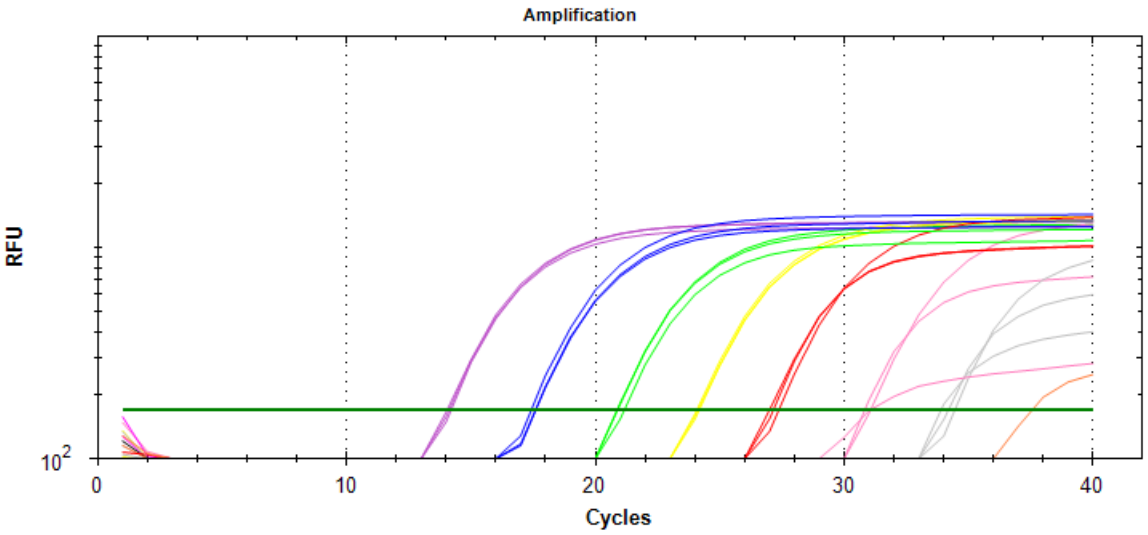


Figure 1: Logarithmic amplification curves for Prunus Necrotic Ringspot Virus

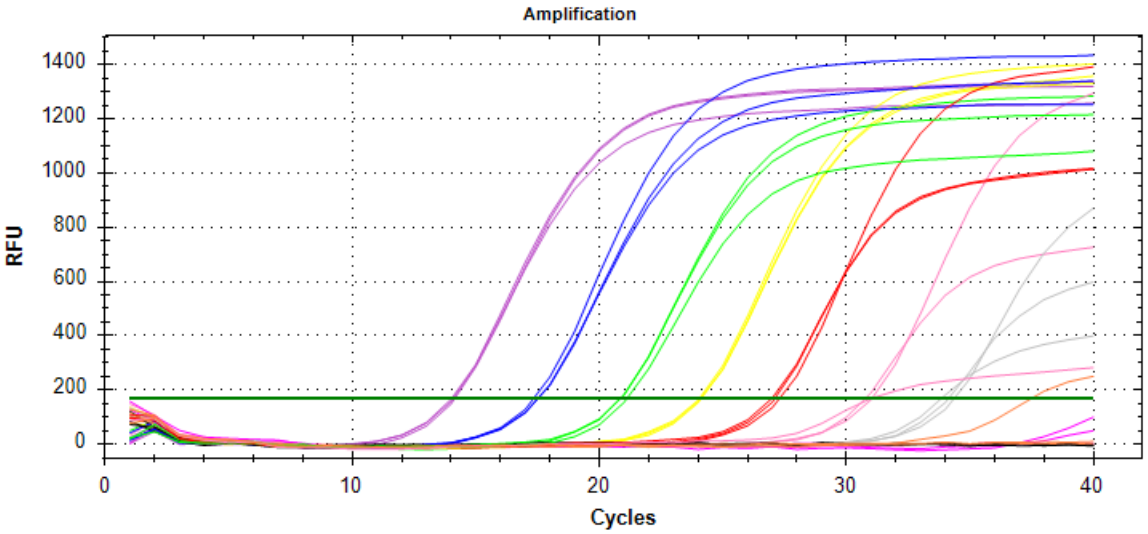


Figure 2: Standard amplification curves for Prunus Necrotic Ringspot Virus

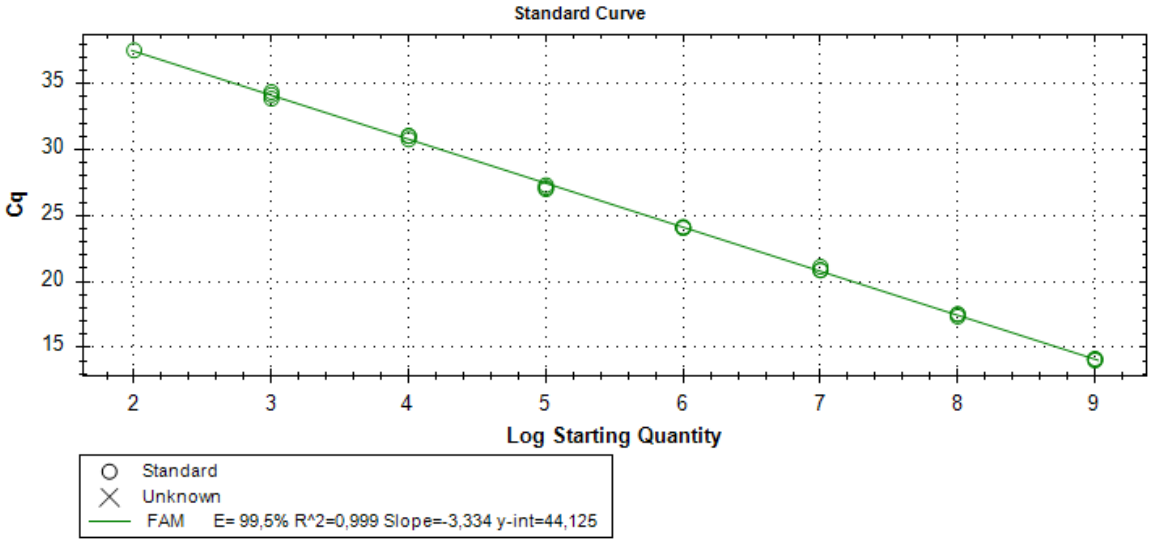


Figure 3: Standard curve for Prunus Necrotic Ringspot Virus

BioinGentech
Biotechnology

Summary of Ct values

Table 2: Ct values obtained for each dilution of the sample control.

Target Name	Sample Name	Reporter	Ct values
Prunus Necrotic Ringspot Virus	**1**	**FAM**	**14,09**
	2	**FAM**	**17,35**
	3	**FAM**	**20,88**
	4	**FAM**	**24,06**
	5	**FAM**	**27,3**
	6	**FAM**	**31,03**
	7	**FAM**	**33,86**
	8	**FAM**	**-**
	Negative Control	**FAM**	Undetermined

Certificate validated by:

BQ. Benjamín Catalán - BQ. Rodrigo Iturra Barra

Quality Control Managers