BioinGentech
Biotechnology

PCR Kit Quality Control Certificate

Pathogen
Thiothrix sp.

Table 1: Concentration in ng/µL of the sample control and its dilutions.

	1	2	3	4	5	6	7	8
	$1x10^{-1}$	$1x10^{-2}$	$1x10^{-3}$	$1x10^{-4}$	$1x10^{-5}$	$1x10^{-6}$	$1x10^{-7}$	$1x10^{-8}$
N° of copies	$1x10^{8}$	$1x10^{7}$	$1x10^{6}$	$1x10^{5}$	$1x10^{4}$	$1x10^{3}$	$1x10^{2}$	$1x10^{1}$

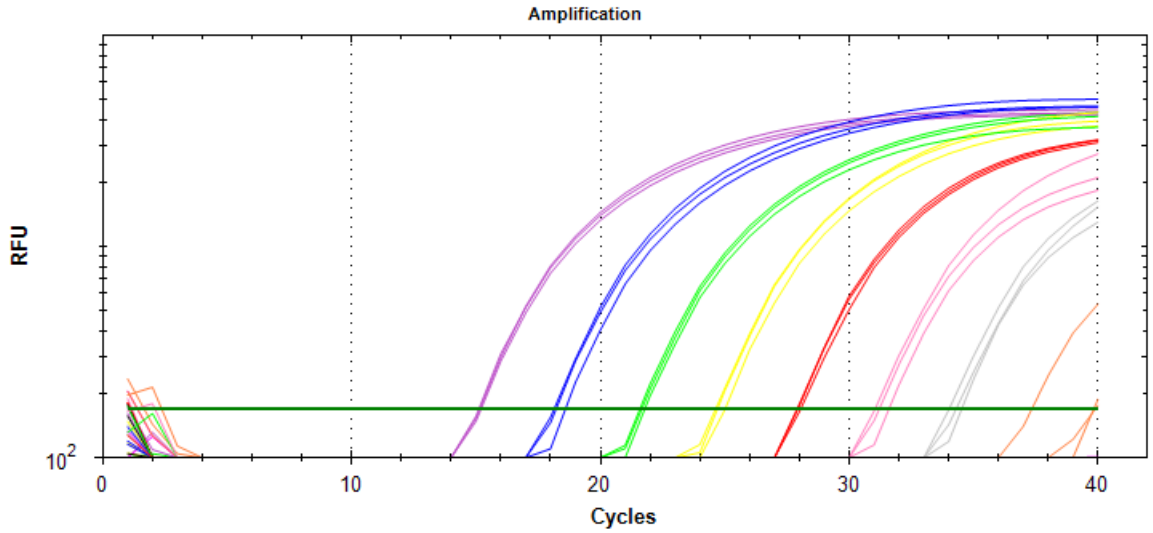

Figure 1: Logarithmic amplification curves for Thiothrix sp.

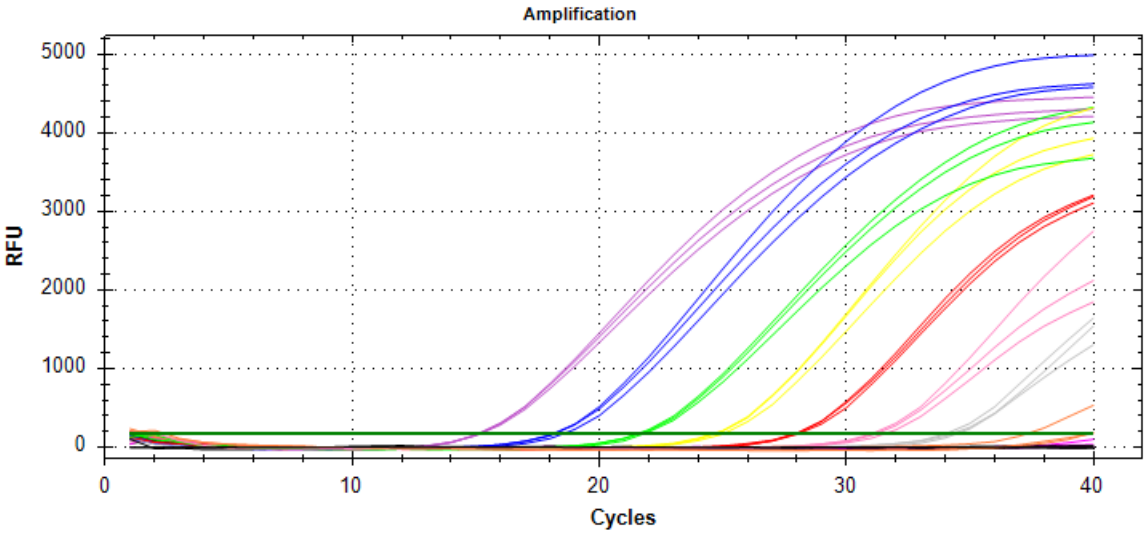

Figure 2: Standard amplification curves for Thiothrix sp.

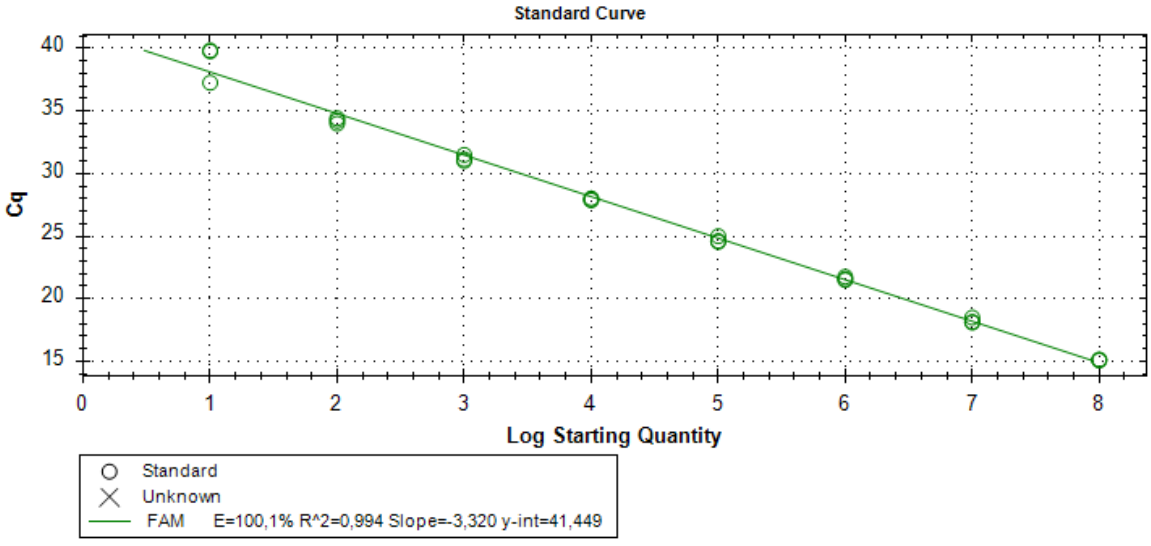

Figure 3: Standard curve for Thiothrix sp.

Summary of Ct values

Table 2: Ct values obtained for each dilution of the sample control.

Target Name	Sample Name	Reporter	Ct values
Thiothrix sp.	1	FAM	15,23
	2	FAM	18,25
	3	FAM	22,82
	4	FAM	26,51
	5	FAM	29,53
	6	FAM	32,11
	7	FAM	35,46
	8	FAM	37,66
	Negative Control	FAM	Undetermined

Certificate validated by:

BQ. Benjamín Catalan - BQ. Rodrigo Iturra Barra

Quality Control Managers